

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time
Kübra Sabit	10.03.2021	09:29:07

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.73 °C
Aerosol	Pressurized air	rel. humidity	2.62 %

Mask information

Mask ID	13868_20210310_092907
Mask los	210309F01001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.80 l/min	39.87 Pa	70.00 Pa	✓ pass
Inhalation 2	94.19 l/min	119.38 Pa	240.00 Pa	✓ pass
Exhalation	159.10 l/min	217.84 Pa	300.00 Pa	✓ pass



Calibration valid until 05.11.2021

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time
Kübra Sabit	10.03.2021	09:32:57

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	93.99 l/min
Generator air	2.97 l/min

Test conditions	
Temperature	21.81 °C
rel. humidity	2.47 %
Mass concentration	19.48 mg/m³


Mask information

Mask ID	13868_20210310_093257
Mask los	210309F01001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 µm)	1.51 %	30.00 %	✓ pass
P_m	0.04 %		
P_Ph_45°	0.11 %	6.00 %	✓ pass

Distributions

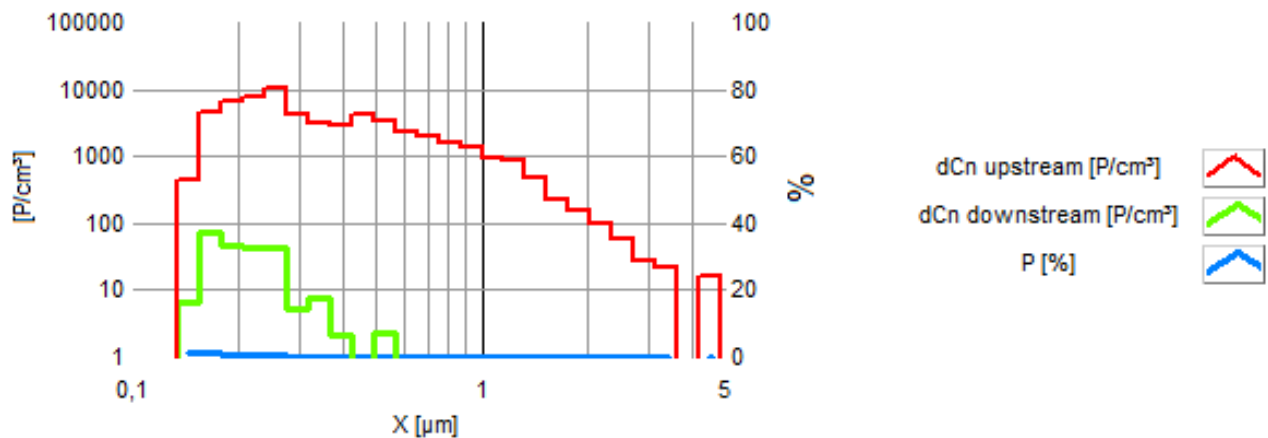

Calibration valid until 05.11.2021