

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time
Kübra Sabit	09.04.2021	08:42:10

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.81 °C
Aerosol	Pressurized air	rel. humidity	3.22 %

Mask information

Mask ID	13868_20210409_084210
Mask los	210408F02001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.72 l/min	42.79 Pa	70.00 Pa	✔ pass
Inhalation 2	94.10 l/min	119.05 Pa	240.00 Pa	✔ pass
Exhalation	159.12 l/min	216.13 Pa	300.00 Pa	✔ pass



Calibration valid until 05.11.2021

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time
Kübra Sabit	09.04.2021	08:52:10

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	93.98 l/min
Generator air	2.97 l/min

Test conditions	
Temperature	21.89 °C
rel. humidity	3.15 %
Mass concentration	21.22 mg/m³


Mask information

Mask ID	13868_20210409_085210
Mask los	210408F02001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 µm)	1.55 %	30.00 %	✓ pass
P_m	0.04 %		
P_Ph_45°	0.10 %	6.00 %	✓ pass

Distributions

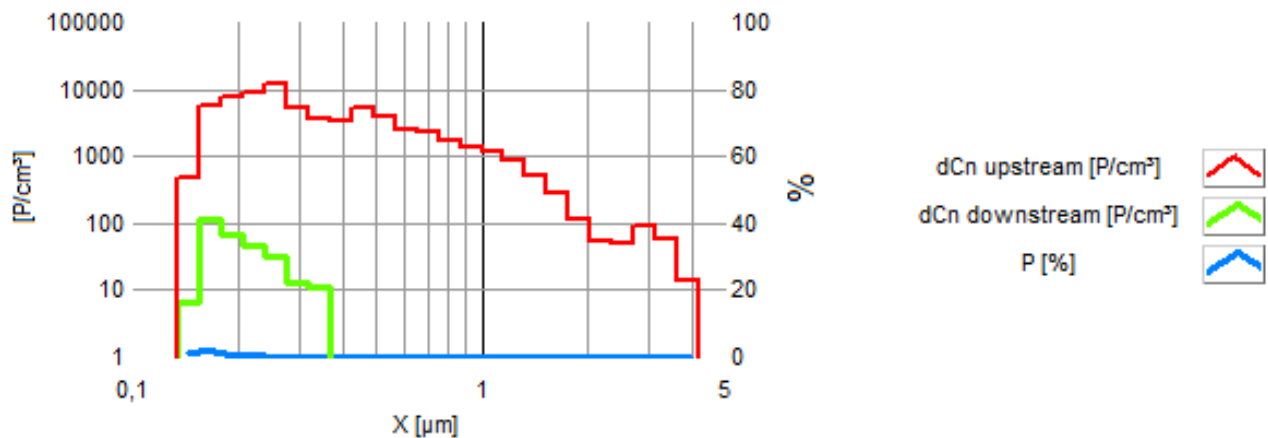

Calibration valid until 05.11.2021