

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time
Kübra Sabit	27.04.2021	08:33:14

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	19.77 °C
Aerosol	Pressurized air	rel. humidity	3.47 %

Mask information

Mask ID	13868_20210427_083314
Mask los	210422F02001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.62 l/min	43.85 Pa	70.00 Pa	✔ pass
Inhalation 2	94.01 l/min	129.90 Pa	240.00 Pa	✔ pass
Exhalation	159.06 l/min	232.99 Pa	300.00 Pa	✔ pass



Calibration valid until 05.11.2021

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time
Kübra Sabit	27.04.2021	08:51:05

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	93.98 l/min
Generator air	2.97 l/min

Test conditions	
Temperature	19.89 °C
rel. humidity	4.56 %
Mass concentration	18.04 mg/m³


Mask information

Mask ID	13868_20210427_085105
Mask los	210422F02001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 µm)	1.39 %	30.00 %	✓ pass
P_m	0.03 %		
P_Ph_45°	0.05 %	6.00 %	✓ pass

Distributions

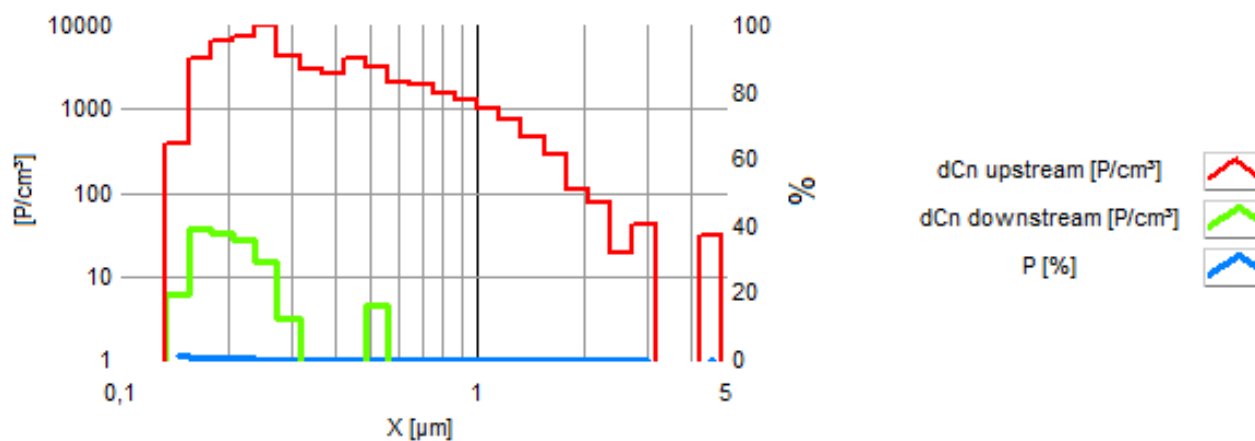

Calibration valid until 05.11.2021