

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time
Kübra Sabit	30.04.2021	08:13:40

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.47 °C
Aerosol	Pressurized air	rel. humidity	2.74 %

Mask information

Mask ID	13868_20210430_081340
Mask los	210429F02001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.69 l/min	40.20 Pa	70.00 Pa	✔ pass
Inhalation 2	94.08 l/min	121.90 Pa	240.00 Pa	✔ pass
Exhalation	159.15 l/min	217.63 Pa	300.00 Pa	✔ pass



Calibration valid until 05.11.2021

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time
Kübra Sabit	30.04.2021	08:17:18

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.00 l/min
Generator air	2.97 l/min

Test conditions	
Temperature	21.54 °C
rel. humidity	4.30 %
Mass concentration	24.37 mg/m³


Mask information

Mask ID	13868_20210430_081718
Mask los	210429F02001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 µm)	2.34 %	30.00 %	✓ pass
P_m	0.51 %		
P_Ph_45°	0.34 %	6.00 %	✓ pass

Distributions

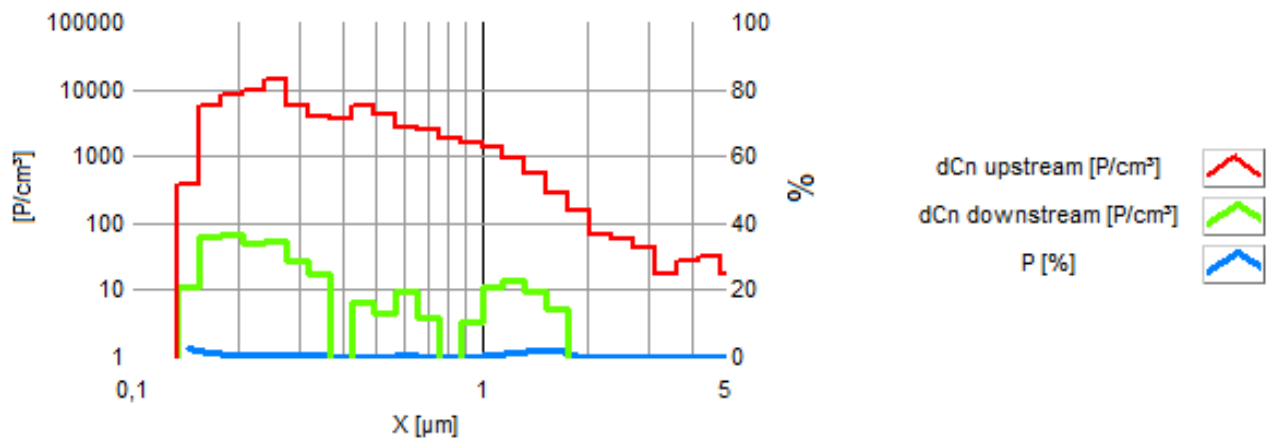

Calibration valid until 05.11.2021