

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Svenja Wilk	09.09.2021	15:58:23	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	27.99 °C
Aerosol	Pressurized air	rel. humidity	3.02 %

Mask information

Mask ID	13868_20210909_155823
Mask lot	20210823-S-L2-002-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.29 l/min	31.99 Pa	70.00 Pa	✔ pass
Inhalation 2	94.87 l/min	113.58 Pa	240.00 Pa	✔ pass
Exhalation	160.08 l/min	207.40 Pa	300.00 Pa	✔ pass

Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Svenja Wilk	09.09.2021	16:06:19	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.83 l/min
Generator air	2.44 l/min

Test conditions	
Temperature	28.08 °C
rel. humidity	2.34 %
Mass concentration	20.49 mg/m ³

Mask information


Mask ID	13868_20210909_160619
Mask lot	20210823-S-L2-002-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	2.32 %	30.00 %	✓ pass
P_m	0.06 %		
P_Ph_45°	0.17 %	6.00 %	✓ pass

Distributions

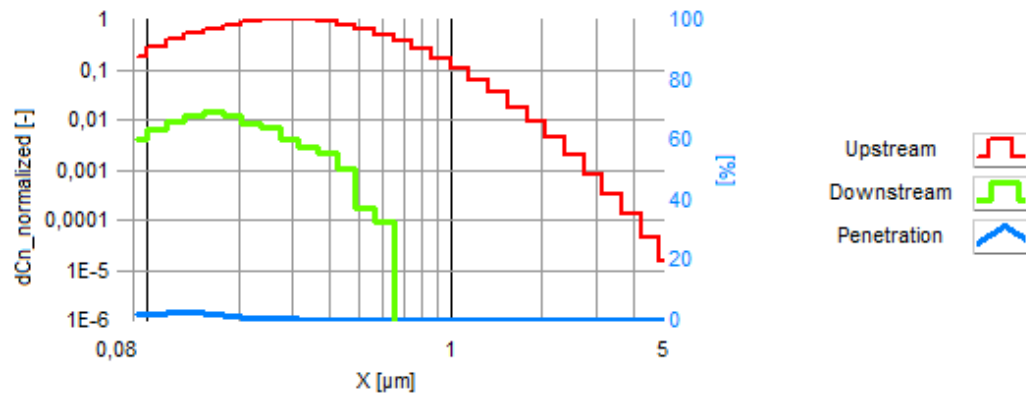

Calibration valid until 03.09.2022