

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Svenja Wilk	26.10.2021	16:35:44	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	24.30 °C
Aerosol	Pressurized air	rel. humidity	3.49 %

Mask information

Mask ID	13868_20211026_163544
Mask lot	20211026-F-L2-002-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.09 l/min	40.75 Pa	70.00 Pa	✔ pass
Inhalation 2	94.84 l/min	127.31 Pa	240.00 Pa	✔ pass
Exhalation	159.98 l/min	219.44 Pa	300.00 Pa	✔ pass

Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Svenja Wilk	26.10.2021	16:40:33	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.96 l/min
Generator air	2.59 l/min

Test conditions	
Temperature	24.18 °C
rel. humidity	2.93 %
Mass concentration	22.10 mg/m³

Mask information


Mask ID	13868_20211026_164033
Mask lot	20211026-F-L2-002-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	0.85 %	30.00 %	✓ pass
P_m	0.09 %		
P_Ph_45°	0.16 %	6.00 %	✓ pass

Distributions

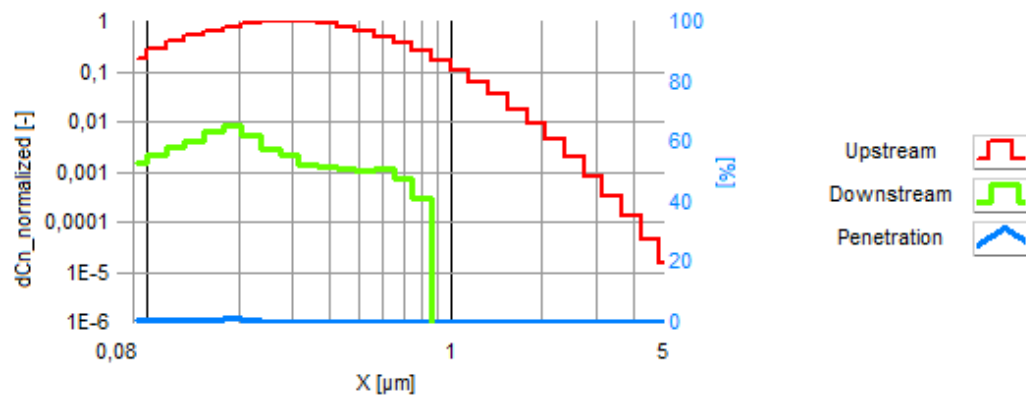

Calibration valid until 03.09.2022