

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Christopher Reinhold	09.12.2021	11:41:36	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	22.91 °C
Aerosol	Pressurized air	rel. humidity	3.03 %

Mask information

Mask ID	13868_20211209_114136
Mask lot	211209-F-L1-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.09 l/min	30.75 Pa	70.00 Pa	✔ pass
Inhalation 2	94.77 l/min	94.48 Pa	240.00 Pa	✔ pass
Exhalation	159.91 l/min	162.04 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Christopher Reinhold	09.12.2021	11:47:05	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.90 l/min
Generator air	3.23 l/min

Test conditions	
Temperature	22.91 °C
rel. humidity	2.52 %
Mass concentration	69.59 mg/m³

Mask information


Mask ID	13868_20211209_114705
Mask lot	211209-F-L1-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	2.11 %	30.00 %	✔ pass
P_m	0.05 %		
P_Ph_45°	0.12 %	6.00 %	✔ pass

Distributions

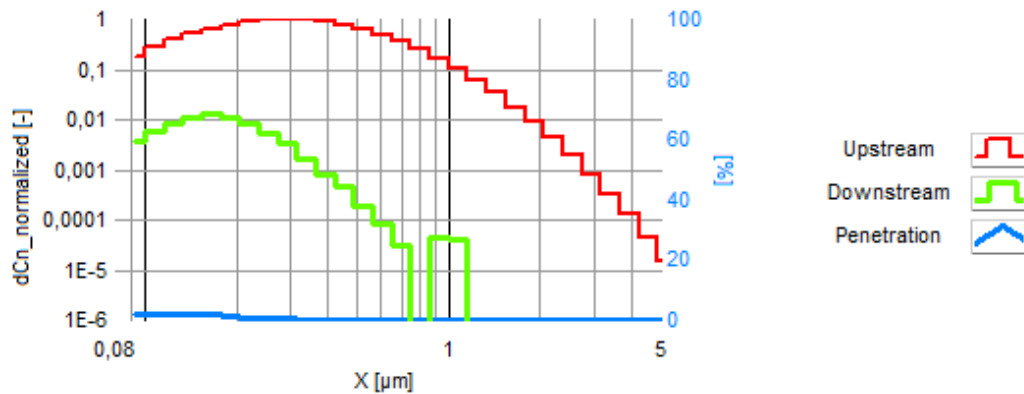

Calibration valid until 03.09.2022