

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	20.12.2021	12:46:20	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	25.25 °C
Aerosol	Pressurized air	rel. humidity	2.49 %

Mask information

Mask ID	13868_20211220_124620
Mask lot	211220-F-L3-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.08 l/min	32.29 Pa	70.00 Pa	✔ pass
Inhalation 2	94.68 l/min	97.14 Pa	240.00 Pa	✔ pass
Exhalation	160.00 l/min	168.16 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	20.12.2021	12:50:29	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.92 l/min
Generator air	2.69 l/min

Test conditions	
Temperature	25.27 °C
rel. humidity	2.15 %
Mass concentration	21.73 mg/m ³

Mask information


Mask ID	13868_20211220_125029
Mask lot	211220-F-L3-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	2.52 %	6.00 %	✓ pass
P_m	0.44 %		
P_Ph_45°	0.58 %	6.00 %	✓ pass

Distributions

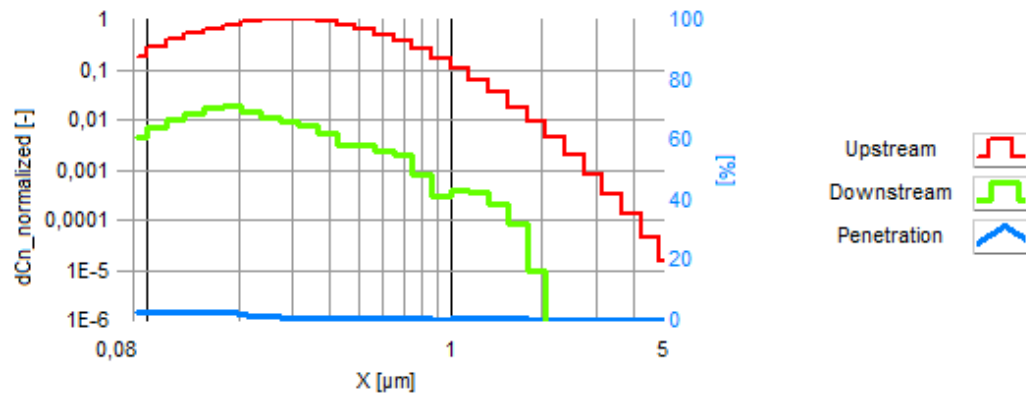

Calibration valid until 03.09.2022