

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad	10.05.2022	11:31:30	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	24.33 °C
Aerosol	Pressurized air	rel. humidity	3.06 %

Mask information

Mask ID	13868_20220510_113130
Mask lot	220509-F-L2-1-K6-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.03 l/min	30.17 Pa	70.00 Pa	✔ pass
Inhalation 2	94.67 l/min	91.49 Pa	240.00 Pa	✔ pass
Exhalation	159.98 l/min	157.84 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad	10.05.2022	11:35:58	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.99 l/min
Generator air	2.62 l/min

Test conditions	
Temperature	24.30 °C
rel. humidity	2.64 %
Mass concentration	20.57 mg/m ³

Mask information


Mask ID	13868_20220510_113558
Mask lot	220509-F-L2-1-K6-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	10.03 %	20.00 %	✔ pass
P_m	0.52 %		
P_Ph_45°	1.09 %	6.00 %	✔ pass

Distributions

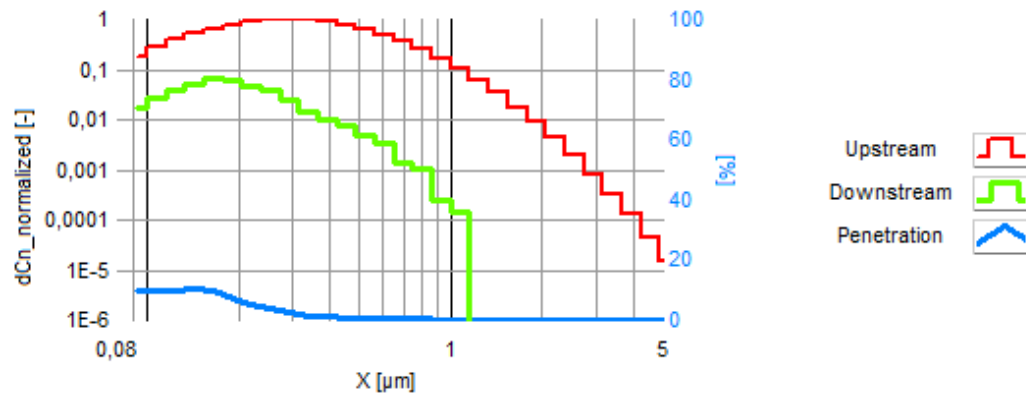

Calibration valid until 03.09.2022