

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	30.03.2022	08:53:43	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	20.37 °C
Aerosol	Pressurized air	rel. humidity	2.93 %

Mask information

Mask ID	13868_20220330_085343
Mask lot	220329-S-L3-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.04 l/min	42.38 Pa	70.00 Pa	✔ pass
Inhalation 2	94.81 l/min	112.25 Pa	240.00 Pa	✔ pass
Exhalation	159.94 l/min	184.46 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	30.03.2022	08:57:15	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.77 l/min
Generator air	2.69 l/min

Test conditions	
Temperature	20.39 °C
rel. humidity	2.75 %
Mass concentration	18.23 mg/m ³

Mask information


Mask ID	13868_20220330_085715
Mask lot	220329-S-L3-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	3.38 %	20.00 %	✓ pass
P_m	0.23 %		
P_Ph_45°	0.32 %	6.00 %	✓ pass

Distributions

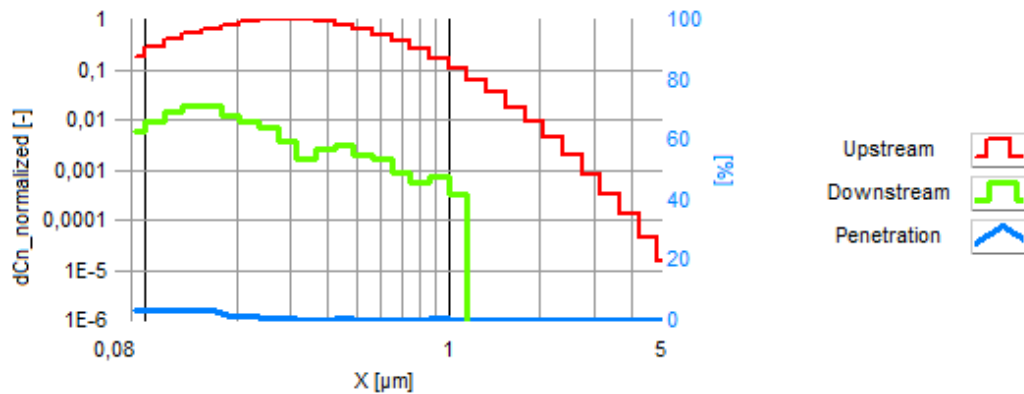

Calibration valid until 03.09.2022