

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	06.04.2022	09:53:41	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	23.39 °C
Aerosol	Pressurized air	rel. humidity	2.84 %

Mask information

Mask ID	13868_20220406_095341
Mask lot	220405-S-L5-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.11 l/min	36.35 Pa	70.00 Pa	✔ pass
Inhalation 2	94.81 l/min	107.07 Pa	240.00 Pa	✔ pass
Exhalation	159.90 l/min	185.19 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	06.04.2022	09:58:16	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.96 l/min
Generator air	2.78 l/min

Test conditions	
Temperature	23.43 °C
rel. humidity	2.32 %
Mass concentration	21.88 mg/m ³

Mask information


Mask ID	13868_20220406_095816
Mask lot	220405-S-L5-2-M2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	1.71 %	20.00 %	✔ pass
P_m	0.06 %		
P_Ph_45°	0.14 %	6.00 %	✔ pass

Distributions

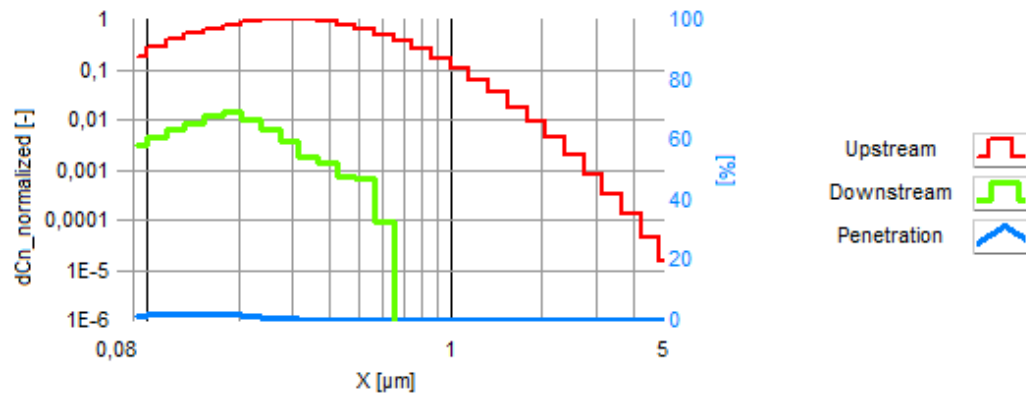

Calibration valid until 03.09.2022