

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	04.01.2022	08:51:32	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.24 °C
Aerosol	Pressurized air	rel. humidity	3.13 %

Mask information

Mask ID	13868_20220104_085132
Mask lot	220104-F-L3-2-M2a-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.12 l/min	37.98 Pa	70.00 Pa	✔ pass
Inhalation 2	94.81 l/min	104.18 Pa	240.00 Pa	✔ pass
Exhalation	160.01 l/min	173.92 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	04.01.2022	08:55:29	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.89 l/min
Generator air	2.68 l/min

Test conditions	
Temperature	21.25 °C
rel. humidity	3.03 %
Mass concentration	19.10 mg/m ³

Mask information


Mask ID	13868_20220104_085529
Mask lot	220104-F-L3-2-M2a-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	3.07 %	6.00 %	✓ pass
P_m	0.48 %		
P_Ph_45°	0.42 %	6.00 %	✓ pass

Distributions

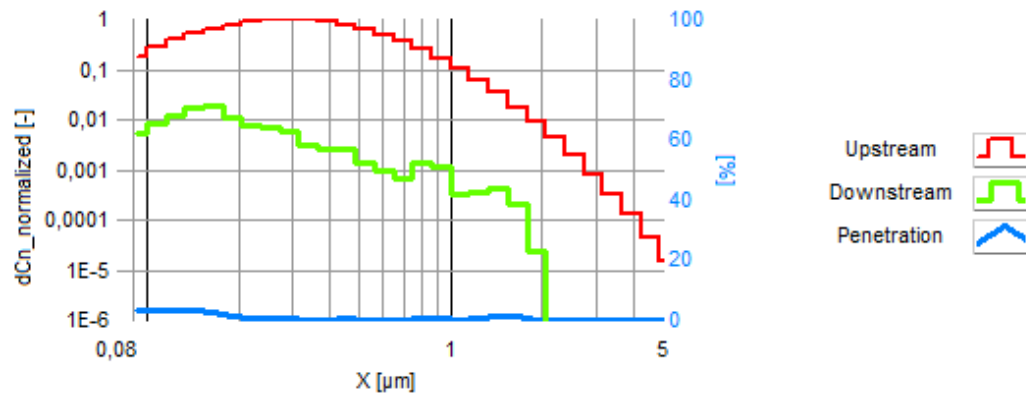

Calibration valid until 03.09.2022