

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	12.01.2022	10:34:42	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	19.88 °C
Aerosol	Pressurized air	rel. humidity	3.81 %

Mask information

Mask ID	13868_20220112_103442
Mask lot	220112-F-L4-2-M2a-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.95 l/min	38.78 Pa	70.00 Pa	✔ pass
Inhalation 2	94.73 l/min	102.20 Pa	240.00 Pa	✔ pass
Exhalation	159.94 l/min	168.18 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	12.01.2022	10:43:26	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.82 l/min
Generator air	2.69 l/min

Test conditions	
Temperature	19.88 °C
rel. humidity	3.27 %
Mass concentration	17.84 mg/m ³

Mask information


Mask ID	13868_20220112_104326
Mask lot	220112-F-L4-2-M2a-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	0.76 %	6.00 %	✓ pass
P_m	0.01 %		
P_Ph_45°	0.02 %	6.00 %	✓ pass

Distributions

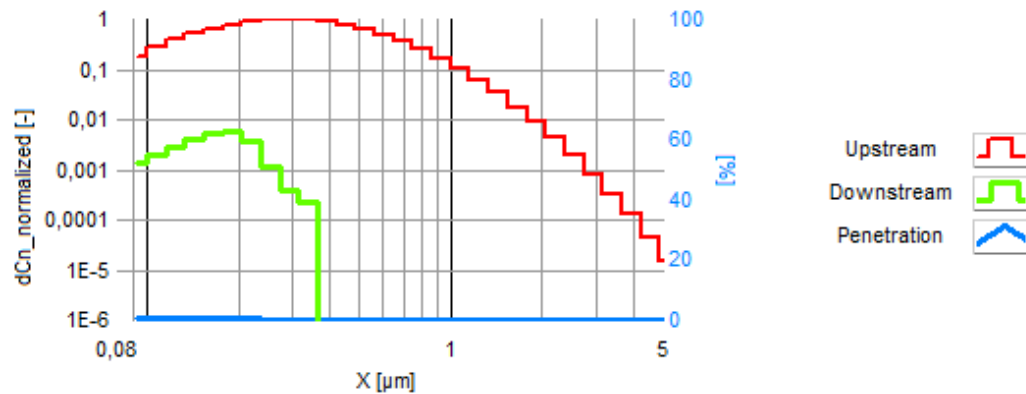

Calibration valid until 03.09.2022