

## Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	04.04.2022	12:21:03	1.11.1.0

### Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	19.79 °C
Aerosol	Pressurized air	rel. humidity	3.77 %

### Mask information

Mask ID	13868_20220404_122103
Mask lot	220404-F-L4-2-M2a-A-IN
Mask type	DMASKE / Chargentest / FFP 2

### Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.03 l/min	33.62 Pa	70.00 Pa	✔ pass
Inhalation 2	94.61 l/min	99.83 Pa	240.00 Pa	✔ pass
Exhalation	159.88 l/min	168.33 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

## Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	04.04.2022	12:27:13	1.11.1.0

### Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.99 l/min
Generator air	2.84 l/min

Test conditions	
Temperature	19.80 °C
rel. humidity	3.13 %
Mass concentration	20.26 mg/m <sup>3</sup>

### Mask information


Mask ID	13868_20220404_122713
Mask lot	220404-F-L4-2-M2a-A-IN
Mask type	DMASKE / Chargentest / FFP 2

### Result

Calculation of the penetration is based on the following parameters:  $X_g = 0.29 \mu\text{m}$ ,  $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 $\mu\text{m}$ )	2.70 %	20.00 %	✔ pass
P_m	0.20 %		
P_Ph_45°	0.28 %	6.00 %	✔ pass

### Distributions

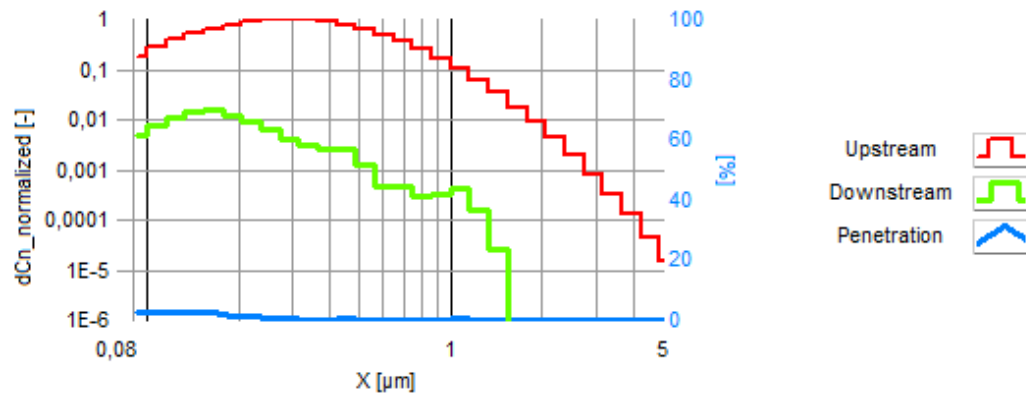

Calibration valid until 03.09.2022