

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	26.09.2022	09:30:51	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.89 l/min
Generator air	2.68 l/min

Test conditions	
Temperature	22.92 °C
rel. humidity	3.50 %
Mass concentration	19.53 mg/m³

Mask information


Mask ID	13868_20220926_093051
Mask lot	220923-F-L4-2-M2a-A-IN_DM
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	1.67 %	20.00 %	✔ pass
P_m	0.06 %		
P_Ph_45°	0.14 %	6.00 %	✔ pass

Distributions

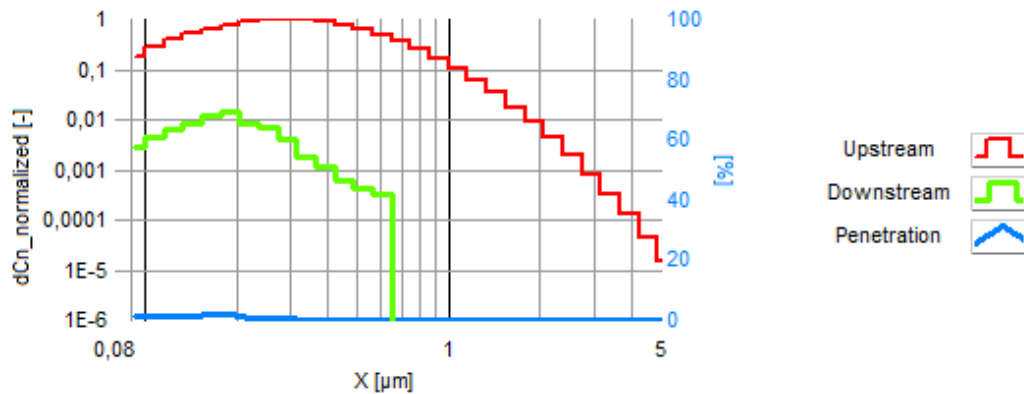

Calibration expired since 03.09.2022

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	26.09.2022	09:27:13	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	22.87 °C
Aerosol	Pressurized air	rel. humidity	2.93 %

Mask information

Mask ID	13868_20220926_092713
Mask lot	220923-F-L4-2-M2a-A-IN_DM
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.21 l/min	32.44 Pa	70.00 Pa	✔ pass
Inhalation 2	94.73 l/min	102.59 Pa	240.00 Pa	✔ pass
Exhalation	159.90 l/min	179.45 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022