

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Carsten	07.10.2022	14:20:53	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	23.98 °C
Aerosol	Pressurized air	rel. humidity	3.57 %

Mask information

Mask ID	13868_20221007_142053
Mask lot	221006-F-L4-2-M2a-A-IN_D
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.06 l/min	18.78 Pa	70.00 Pa	✔ pass
Inhalation 2	94.82 l/min	78.69 Pa	240.00 Pa	✔ pass
Exhalation	159.91 l/min	142.98 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Carsten	07.10.2022	14:32:40	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.99 l/min
Generator air	2.63 l/min

Test conditions	
Temperature	23.95 °C
rel. humidity	3.61 %
Mass concentration	18.70 mg/m³

Mask information


Mask ID	13868_20221007_143240
Mask lot	221006-F-L4-2-M2a-B-IN_D
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	3.93 %	20.00 %	✔ pass
P_m	0.56 %		
P_Ph_45°	0.30 %	6.00 %	✔ pass

Distributions

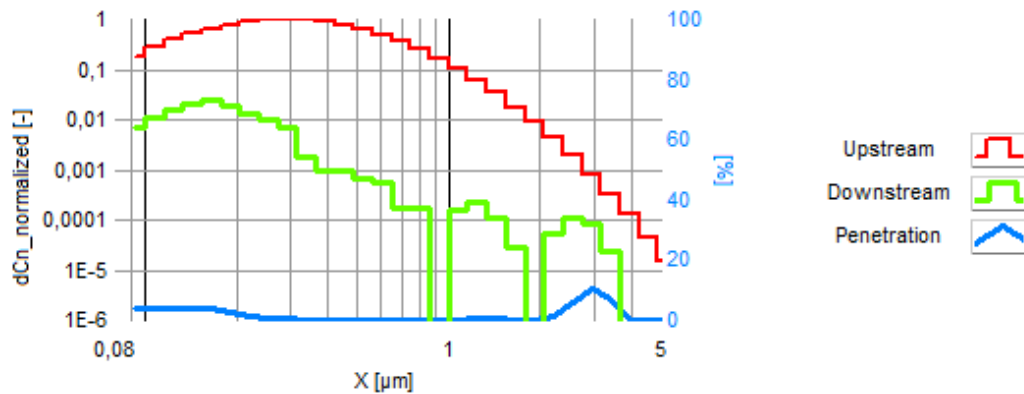

Calibration expired since 03.09.2022