

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Carsten	07.10.2022	15:51:18	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	25.15 °C
Aerosol	Pressurized air	rel. humidity	2.15 %

Mask information

Mask ID	13868_20221007_155118
Mask lot	221007-F-L3-2-M2a-A-IN_D
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.02 l/min	24.97 Pa	70.00 Pa	✔ pass
Inhalation 2	94.79 l/min	88.49 Pa	240.00 Pa	✔ pass
Exhalation	160.03 l/min	159.34 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Carsten	07.10.2022	15:56:37	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.95 l/min
Generator air	2.59 l/min

Test conditions	
Temperature	25.25 °C
rel. humidity	2.94 %
Mass concentration	18.17 mg/m ³

Mask information


Mask ID	13868_20221007_155637
Mask lot	221007-F-L3-2-M2a-A-IN_D
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	3.47 %	20.00 %	✔ pass
P_m	0.06 %		
P_Ph_45°	0.15 %	6.00 %	✔ pass

Distributions

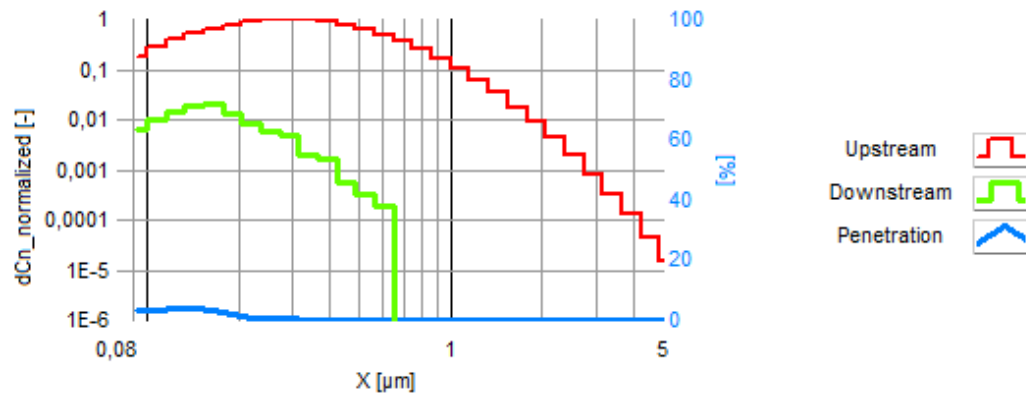

Calibration expired since 03.09.2022