

## Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	17.10.2022	13:03:22	1.11.1.0

### Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.88 l/min
Generator air	2.53 l/min

Test conditions	
Temperature	25.25 °C
rel. humidity	3.61 %
Mass concentration	21.54 mg/m <sup>3</sup>

### Mask information


Mask ID	13868_20221017_130322
Mask lot	221014-S-L3-2-M2a-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

### Result

Calculation of the penetration is based on the following parameters:  $X_g = 0.29 \mu\text{m}$ ,  $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 $\mu\text{m}$ )	1.64 %	20.00 %	✔ pass
P_m	0.03 %		
P_Ph_45°	0.06 %	6.00 %	✔ pass

### Distributions

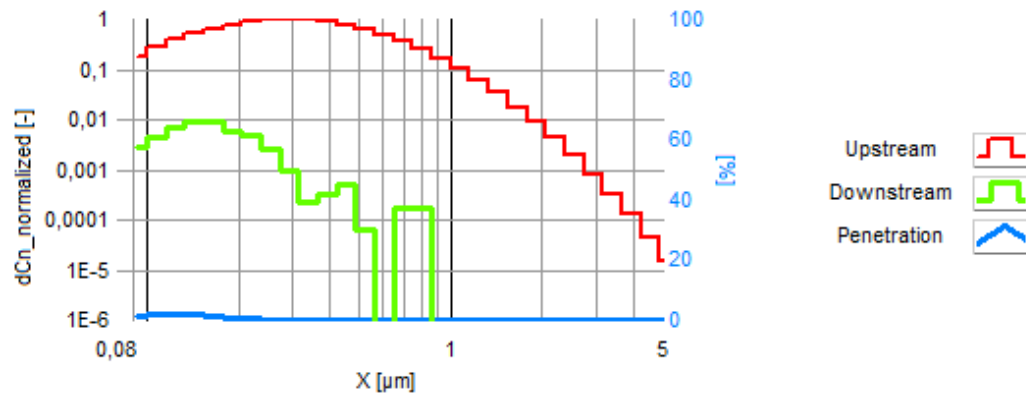

Calibration expired since 03.09.2022

## Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	17.10.2022	12:59:54	1.11.1.0

### Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	25.25 °C
Aerosol	Pressurized air	rel. humidity	3.23 %

### Mask information

Mask ID	13868_20221017_125954
Mask lot	221014-S-L3-2-M2a-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

### Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.08 l/min	28.51 Pa	70.00 Pa	✔ pass
Inhalation 2	94.89 l/min	101.37 Pa	240.00 Pa	✔ pass
Exhalation	159.97 l/min	179.88 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022