

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	31.10.2022	11:03:33	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.86 l/min
Generator air	2.68 l/min

Test conditions	
Temperature	23.87 °C
rel. humidity	2.71 %
Mass concentration	21.18 mg/m ³

Mask information


Mask ID	13868_20221031_110333
Mask lot	221027-S-L4-2-M2A-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	0.70 %	20.00 %	✔ pass
P_m	0.03 %		
P_Ph_45°	0.08 %	6.00 %	✔ pass

Distributions

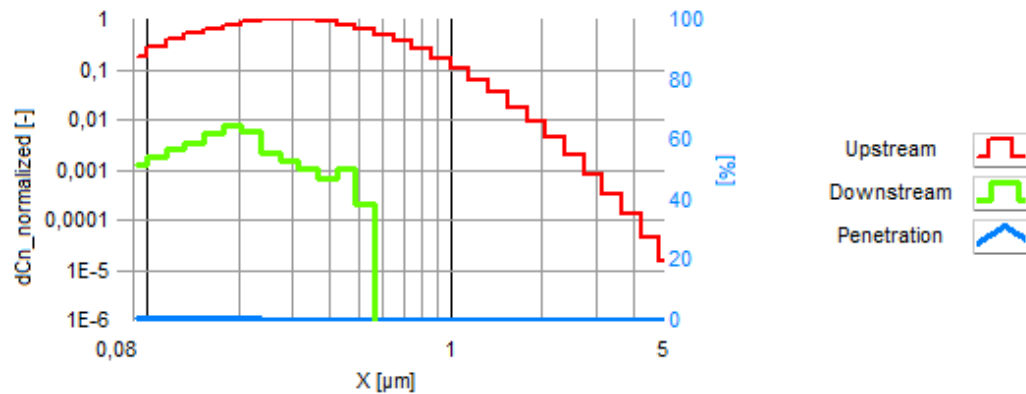

Calibration expired since 03.09.2022

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	31.10.2022	11:00:09	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	23.88 °C
Aerosol	Pressurized air	rel. humidity	3.28 %

Mask information

Mask ID	13868_20221031_110009
Mask lot	221027-S-L4-2-M2A-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.03 l/min	35.96 Pa	70.00 Pa	✔ pass
Inhalation 2	94.80 l/min	111.42 Pa	240.00 Pa	✔ pass
Exhalation	159.93 l/min	192.26 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022