

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	04.11.2022	15:20:26	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.84 l/min
Generator air	2.68 l/min

Test conditions	
Temperature	21.93 °C
rel. humidity	2.84 %
Mass concentration	22.09 mg/m ³

Mask information


Mask ID	13868_20221104_152026
Mask lot	221103-S-L2-2-M2A-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	1.09 %	20.00 %	✓ pass
P_m	0.04 %		
P_Ph_45°	0.09 %	6.00 %	✓ pass

Distributions

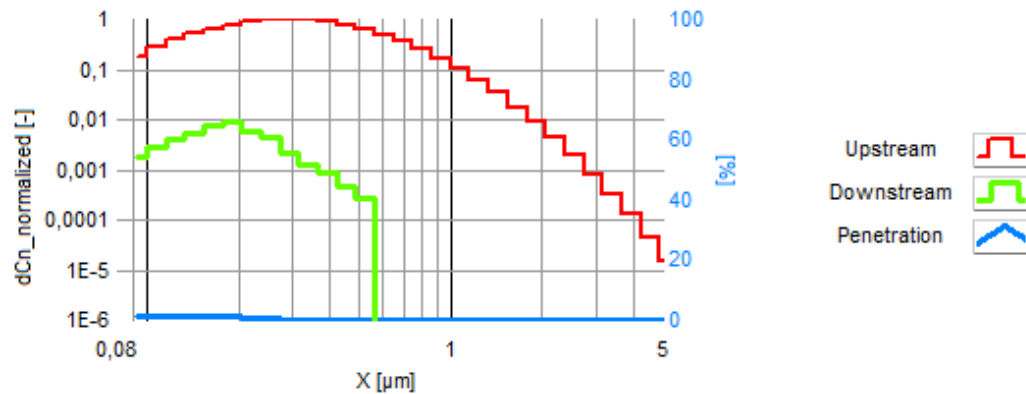

Calibration expired since 03.09.2022

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	04.11.2022	15:16:39	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.83 °C
Aerosol	Pressurized air	rel. humidity	3.02 %

Mask information

Mask ID	13868_20221104_151639
Mask lot	221103-S-L2-2-M2A-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.11 l/min	29.50 Pa	70.00 Pa	✔ pass
Inhalation 2	94.84 l/min	102.29 Pa	240.00 Pa	✔ pass
Exhalation	160.00 l/min	179.07 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022