

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad	30.06.2022	11:17:32	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	23.98 °C
Aerosol	Pressurized air	rel. humidity	9.30 %

Mask information

Mask ID	13868_20220630_111732
Mask lot	220627-F-L4-2-M2b-BL-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.17 l/min	28.63 Pa	70.00 Pa	✔ pass
Inhalation 2	94.76 l/min	101.32 Pa	240.00 Pa	✔ pass
Exhalation	160.05 l/min	175.78 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad	30.06.2022	11:22:13	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.89 l/min
Generator air	2.53 l/min

Test conditions	
Temperature	24.06 °C
rel. humidity	8.92 %
Mass concentration	18.25 mg/m ³

Mask information


Mask ID	13868_20220630_112213
Mask lot	220627-F-L4-2-M2b-BL-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	2.83 %	20.00 %	✓ pass
P_m	0.04 %		
P_Ph_45°	0.08 %	6.00 %	✓ pass

Distributions

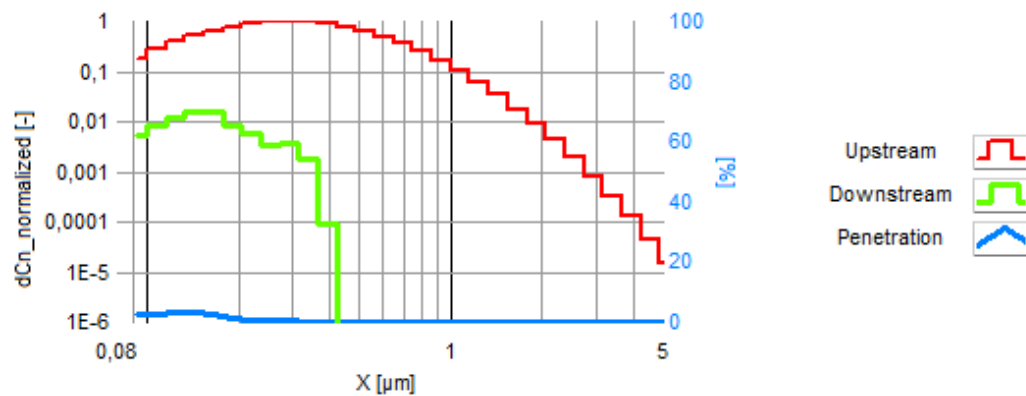

Calibration valid until 03.09.2022