

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	04.11.2022	14:58:20	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.85 l/min
Generator air	2.68 l/min

Test conditions	
Temperature	21.65 °C
rel. humidity	3.08 %
Mass concentration	21.61 mg/m³

Mask information


Mask ID	13868_20221104_145820
Mask lot	221102-S-L6-2-MLK-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	5.23 %	20.00 %	✔ pass
P_m	0.20 %		
P_Ph_45°	0.44 %	6.00 %	✔ pass

Distributions

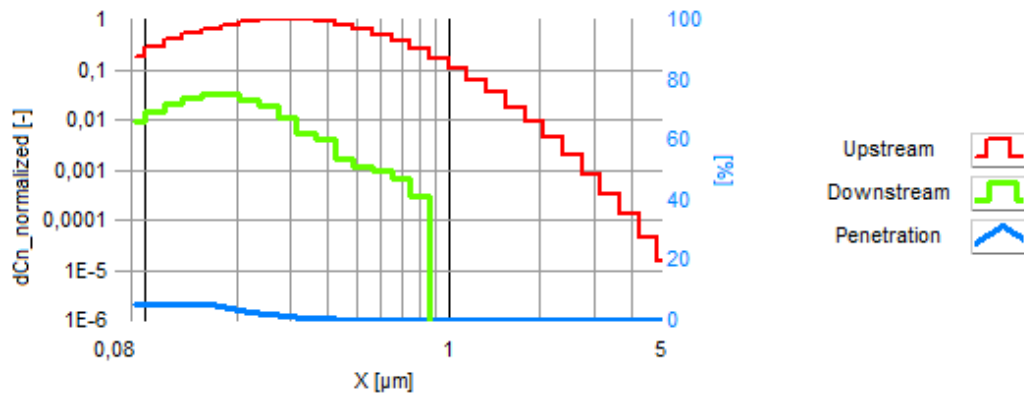

Calibration expired since 03.09.2022

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	04.11.2022	14:53:31	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.61 °C
Aerosol	Pressurized air	rel. humidity	3.52 %

Mask information

Mask ID	13868_20221104_145331
Mask lot	221102-S-L6-2-MLK-A-IN_D_
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.07 l/min	31.01 Pa	70.00 Pa	✔ pass
Inhalation 2	94.80 l/min	112.43 Pa	240.00 Pa	✔ pass
Exhalation	159.97 l/min	214.34 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022