

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Saad Benchakroun	11.04.2022	09:21:51	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	22.61 °C
Aerosol	Pressurized air	rel. humidity	2.52 %

Mask information

Mask ID	13868_20220411_092151
Mask lot	220407-S-L5-2-MLK-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.05 l/min	34.08 Pa	70.00 Pa	✔ pass
Inhalation 2	94.65 l/min	100.79 Pa	240.00 Pa	✔ pass
Exhalation	160.06 l/min	174.55 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Saad Benchakroun	11.04.2022	09:26:07	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	95.00 l/min
Generator air	2.84 l/min

Test conditions	
Temperature	22.61 °C
rel. humidity	2.25 %
Mass concentration	19.88 mg/m ³

Mask information


Mask ID	13868_20220411_092607
Mask lot	220407-S-L5-2-MLK-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	2.16 %	20.00 %	✓ pass
P_m	0.23 %		
P_Ph_45°	0.23 %	6.00 %	✓ pass

Distributions

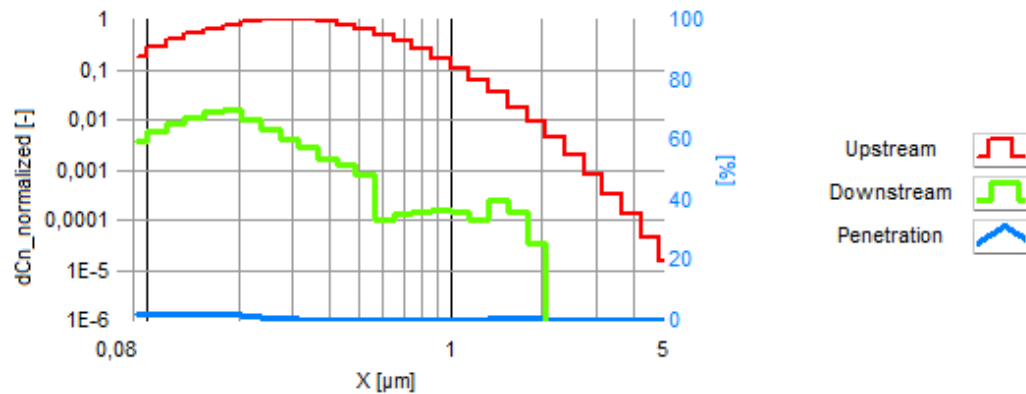

Calibration valid until 03.09.2022