

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Carsten	27.05.2022	09:22:58	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	21.93 °C
Aerosol	Pressurized air	rel. humidity	3.32 %

Mask information

Mask ID	13868_20220527_092258
Mask lot	220524-F-L5-2-LK-A-IN_D
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.05 l/min	33.76 Pa	70.00 Pa	✔ pass
Inhalation 2	94.81 l/min	102.48 Pa	240.00 Pa	✔ pass
Exhalation	159.93 l/min	178.04 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Carsten	27.05.2022	09:27:30	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.85 l/min
Generator air	2.69 l/min

Test conditions	
Temperature	22.00 °C
rel. humidity	3.03 %
Mass concentration	18.94 mg/m ³

Mask information


Mask ID	13868_20220527_092730
Mask lot	220524-F-L5-2-LK-A-IN_D
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	3.21 %	20.00 %	✔ pass
P_m	0.08 %		
P_Ph_45°	0.18 %	6.00 %	✔ pass

Distributions

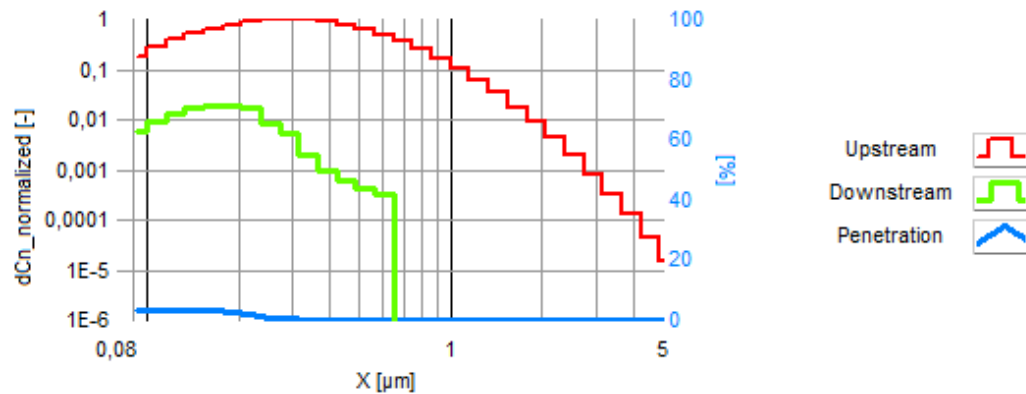

Calibration valid until 03.09.2022