

## Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Asijat Gotschiyaeva	21.06.2022	13:48:17	1.11.1.0

### Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	24.30 °C
Aerosol	Pressurized air	rel. humidity	9.20 %

### Mask information

Mask ID	13868_20220621_134817
Mask lot	220614-F-L5-2-MLK-A-IN
Mask type	DMASKE / Chargentest / FFP 2

### Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.33 l/min	30.09 Pa	70.00 Pa	✔ pass
Inhalation 2	94.71 l/min	108.04 Pa	240.00 Pa	✔ pass
Exhalation	160.02 l/min	177.00 Pa	300.00 Pa	✔ pass



Calibration valid until 03.09.2022

## Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Asijat Gotschiyaeva	21.06.2022	13:52:34	1.11.1.0

### Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.89 l/min
Generator air	2.53 l/min

Test conditions	
Temperature	24.37 °C
rel. humidity	8.69 %
Mass concentration	20.82 mg/m <sup>3</sup>

### Mask information


Mask ID	13868_20220621_135234
Mask lot	220614-F-L5-2-MLK-A-IN
Mask type	DMASKE / Chargentest / FFP 2

### Result

Calculation of the penetration is based on the following parameters:  $X_g = 0.29 \mu\text{m}$ ,  $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 $\mu\text{m}$ )	2.74 %	20.00 %	✔ pass
P_m	0.52 %		
P_Ph_45°	0.31 %	6.00 %	✔ pass

### Distributions

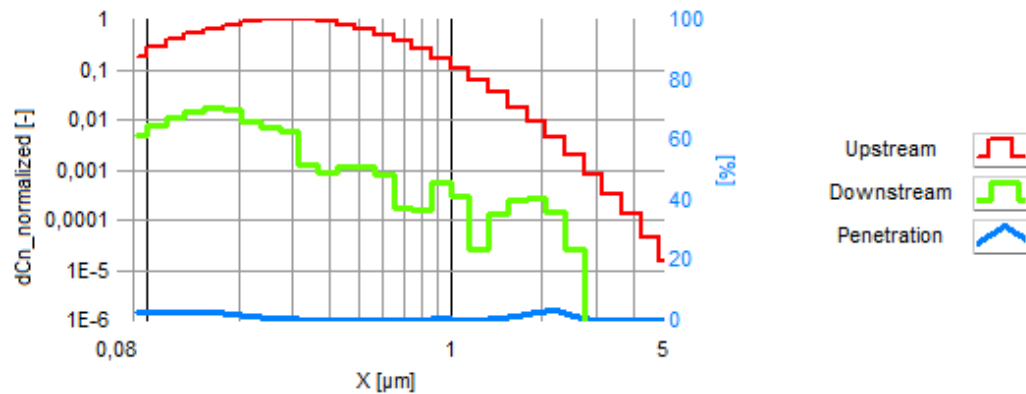

Calibration valid until 03.09.2022