

# Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	15.09.2022	15:28:40	1.11.1.0

## Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.89 l/min
Generator air	2.53 l/min

Test conditions	
Temperature	25.74 °C
rel. humidity	3.03 %
Mass concentration	19.84 mg/m³

## Mask information


Mask ID	13868_20220915_152840
Mask lot	220915-F-L5-2-MLK-A-IN_DM
Mask type	DMASKE / Chargentest / FFP 2

## Result

Calculation of the penetration is based on the following parameters:  $X_g = 0.29 \mu\text{m}$ ,  $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 $\mu\text{m}$ )	4.88 %	20.00 %	✔ pass
P_m	0.21 %		
P_Ph_45°	0.35 %	6.00 %	✔ pass

## Distributions

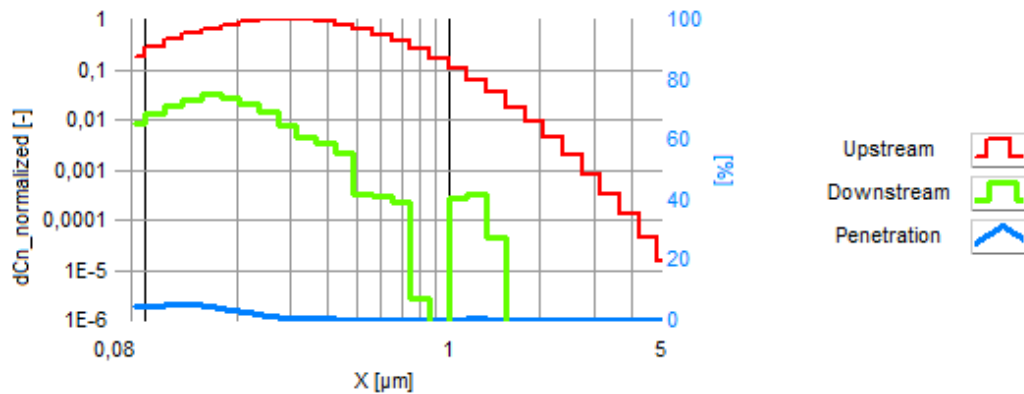

Calibration expired since 03.09.2022

## Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	15.09.2022	15:25:01	1.11.1.0

### Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	25.74 °C
Aerosol	Pressurized air	rel. humidity	2.65 %

### Mask information

Mask ID	13868_20220915_152501
Mask lot	220915-F-L5-2-MLK-A-IN_DM
Mask type	DMASKE / Chargentest / FFP 2

### Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.13 l/min	31.39 Pa	70.00 Pa	✔ pass
Inhalation 2	94.74 l/min	112.41 Pa	240.00 Pa	✔ pass
Exhalation	160.03 l/min	207.97 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022