

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Hikmet	17.11.2022	14:23:48	1.11.1.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.92 l/min
Generator air	2.59 l/min

Test conditions	
Temperature	23.61 °C
rel. humidity	2.64 %
Mass concentration	19.07 mg/m ³

Mask information


Mask ID	13868_20221117_142348
Mask lot	221115-S-L5-MLK-2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	4.54 %	20.00 %	✔ pass
P_m	0.13 %		
P_Ph_45°	0.29 %	6.00 %	✔ pass

Distributions

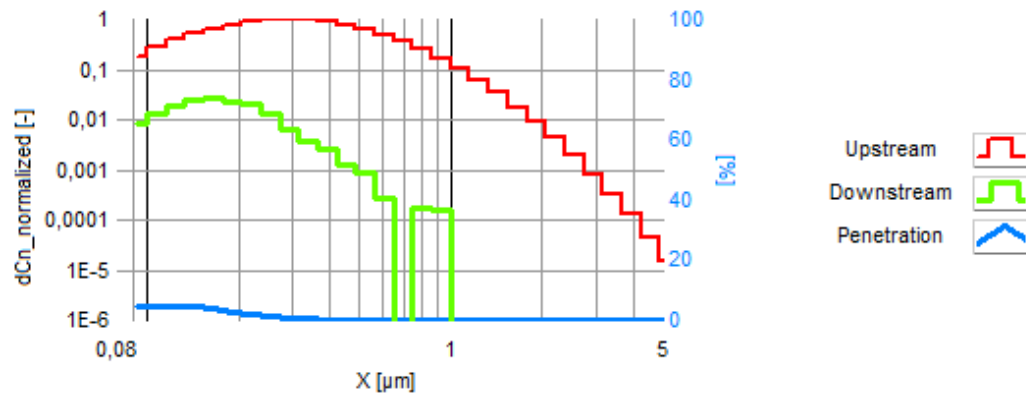

Calibration expired since 03.09.2022

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Hikmet	17.11.2022	14:17:47	1.11.1.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand	Temperature	23.59 °C
Aerosol	Pressurized air	rel. humidity	3.30 %

Mask information

Mask ID	13868_20221117_141747
Mask lot	221115-S-L5-MLK-2-A-IN
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.10 l/min	35.02 Pa	70.00 Pa	✔ pass
Inhalation 2	94.82 l/min	118.70 Pa	240.00 Pa	✔ pass
Exhalation	159.93 l/min	228.81 Pa	300.00 Pa	✔ pass



Calibration expired since 03.09.2022