

Test report - PMFT 1000 - Oil penetration

Operator	Date	Time	Vesion
Dustin	28.02.2023	11:25:55	1.12.0.0

Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	94.51 l/min
Generator air	2.69 l/min

Test conditions	
Temperature	17.63 °C
rel. humidity	4.88 %
Mass concentration	20.41 mg/m³

Mask information


Mask ID	13868_20230228_112555
Mask lot	230227-F-L6-MLK-A-IN_DMAS
Mask type	DMASKE / Chargentest / FFP 2

Result

Calculation of the penetration is based on the following parameters: $X_g = 0.29 \mu\text{m}$, $\text{Sigma} = 1.85$

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 μm)	7.68 %	20.00 %	✓ pass
P_m	0.05 %		
P_Ph_45°	0.09 %	6.00 %	✓ pass

Distributions

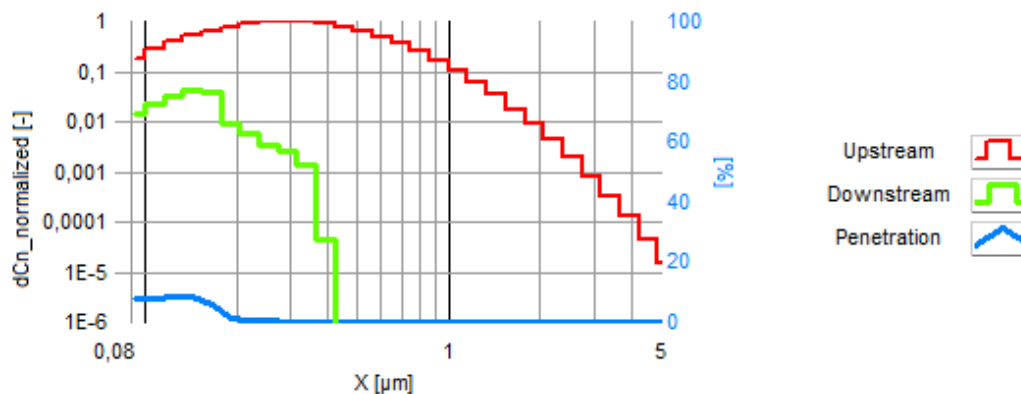

Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time	Vesion
Dustin	28.02.2023	11:23:48	1.12.0.0

Basic information

Operation parameter		Test conditions	
Script	Atemwiderstand 2.0	Temperature	17.53 °C
Aerosol	Pressurized air	rel. humidity	4.99 %

Mask information

Mask ID	13868_20230228_112348
Mask lot	230227-F-L6-MLK-A-IN_DMAS
Mask type	DMASKE / Chargentest / FFP 2

Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	30.04 l/min	32.75 Pa	70.00 Pa	✓ pass
Inhalation 2	94.71 l/min	104.00 Pa	240.00 Pa	✓ pass
Exhalation	NaN l/min	NaN Pa	300.00 Pa	? not tested



Calibration valid until 15.12.2023