

## Test report - PMFT 1000 - Oil penetration

Operator	Date	Time
Jan Thomanek	01.02.2021	19:00:18

### Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	93.99 l/min
Generator air	2.97 l/min

Test conditions	
Temperature	0.00 °C
rel. humidity	0.00 %
Mass concentration	24.75 mg/m <sup>3</sup>


### Mask information

Mask ID	13868_20210201_190018
Mask los	210201S01001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

### Result

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 µm)	4.04 %	30.00 %	✓ pass
P_m	0.08 %		
P_Ph_45°	0.14 %	6.00 %	✓ pass

### Distributions

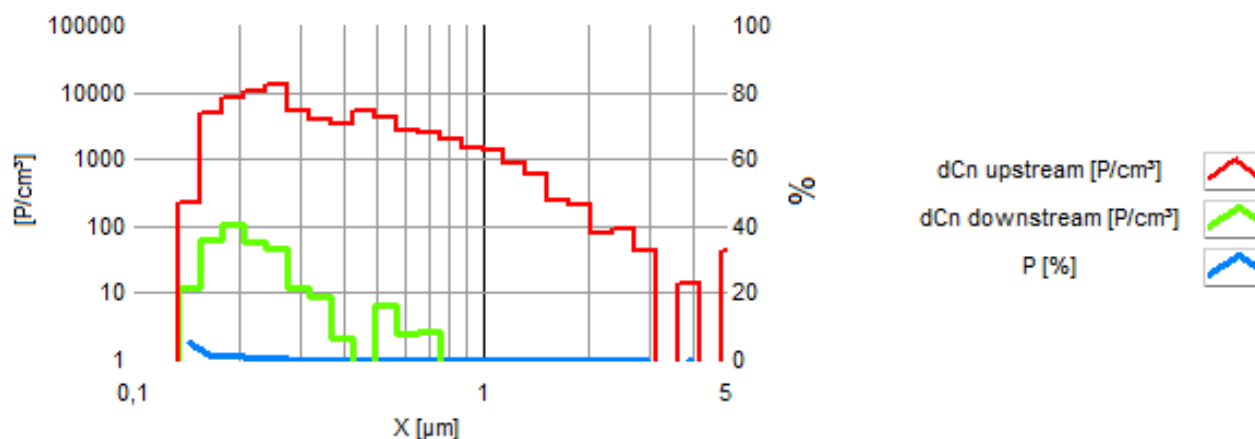

Calibration valid until 05.11.2021

**Test report - PMFT 1000 - Breath resistance / Valve test**

Operator	Date	Time
Jan Thomanek	01.02.2021	18:56:33

**Basic information**

Operation parameter	
Script	Atemwiderstand
Aerosol	Pressurized air

**Mask information**

Mask ID	13868_20210201_185633
Mask los	210201S01001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

**Result**

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.77 l/min	40.31 Pa	70.00 Pa	✔ pass
Inhalation 2	94.19 l/min	123.01 Pa	240.00 Pa	✔ pass
Exhalation	159.05 l/min	215.91 Pa	300.00 Pa	✔ pass



Calibration valid until 05.11.2021