

## Test report - PMFT 1000 - Breath resistance / Valve test

Operator	Date	Time
Jan Thomanek	15.02.2021	10:36:01

### Basic information

Operation parameter	
Script	Atemwiderstand
Aerosol	Pressurized air

### Mask information

Mask ID	13868_20210215_103601
Mask los	210211N01001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

### Result

Description	Main air	Differential pressure	Upper limit	Result
Inhalation 1	29.61 l/min	39.44 Pa	70.00 Pa	✔ pass
Inhalation 2	94.12 l/min	116.63 Pa	240.00 Pa	✔ pass
Exhalation	159.00 l/min	214.58 Pa	300.00 Pa	✔ pass



Calibration valid until 05.11.2021

# Test report - PMFT 1000 - Oil penetration

Operator	Date	Time
Jan Thomanek	15.02.2021	10:40:16

## Basic information

Operation parameter	
Script	Effizienz Test (Öl)
Aerosol	Oil
Main air	93.98 l/min
Generator air	2.97 l/min

Test conditions	
Temperature	0.00 °C
rel. humidity	0.00 %
Mass concentration	18.27 mg/m <sup>3</sup>


## Mask information

Mask ID	13868_20210215_104016
Mask los	210211N01001-A-IN
Mask type	DMASKE / Chargentest / FFP 2

## Result

Penetration	Measurement	Upper limit	Result
P_SARS_CoV-2 (0.15 µm)	0.64 %	30.00 %	✓ pass
P_m	0.05 %		
P_Ph_45°	0.13 %	6.00 %	✓ pass

## Distributions

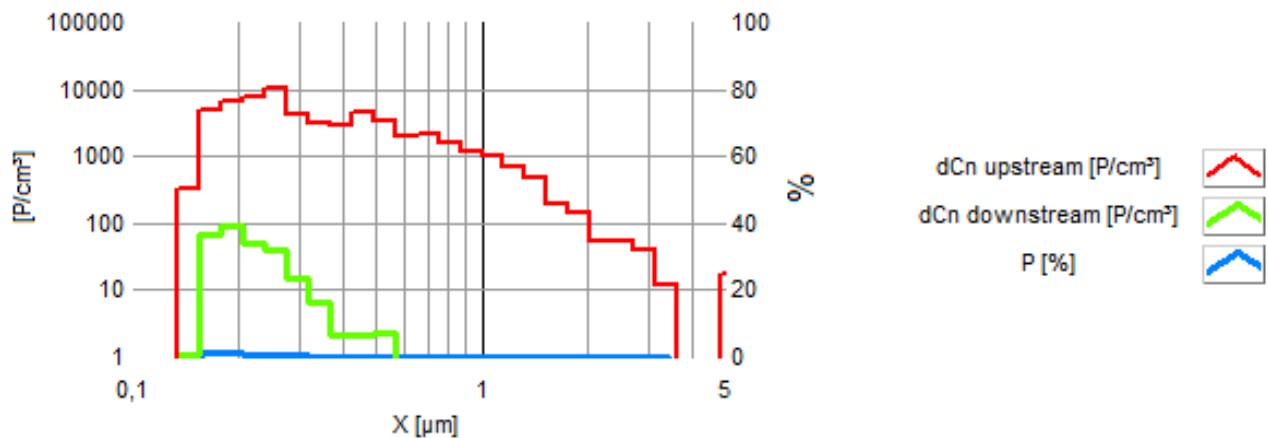

Calibration valid until 05.11.2021